


EXmatic 470

TECHNICAL INFORMATION

Control unit
for retractable probe housings

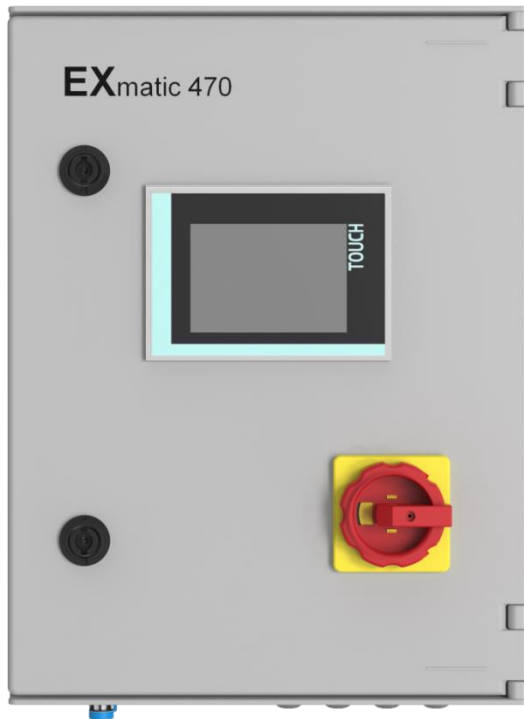

All brand and product names are trademarks of the company:

EXNER PROCESS EQUIPMENT GmbH

Imprint

Distributed by:

Exner Process Equipment GmbH

Carl-Metz-Str. 26

D-76275 Ettlingen

Date of issue: 2022-04-28

As per: 28.04.2022

File: EXmatic 470 TI en 220428

© 2020, Dipl.-Ing. [Graduate Engineer] Detlef Exner

All rights reserved, including the translation.

The reproduction of the content in these operating instructions is subject to prior written approval by EXNER PROCESS EQUIPMENT GMBH, ETTLINGEN.

All technical information, drawings, etc. are subject to the protection of copyright law.

Technical modifications reserved.

Printed on chlorine-free and acid-free pulp paper.

Table of contents

1	Technical data	4
1.1	Standards and directives.....	4
1.2	Material properties.....	4
1.3	Pneumatics.....	4
1.4	Dimensions.....	4
1.5	Environmental conditions.....	5
1.6	Connection values.....	5
1.7	Cleaning valves (optional).....	5
1.8	Identification plate.....	6
2	Product description	7
2.1	EXmatic 470 electro-pneumatic control unit.....	7
2.2	Process integration.....	9
3	EXmatic 470 order structure	12
4	Spare parts and accessories	13
5	Certificates and compliance	14

1 Technical data

1.1 Standards and directives

The following directives were applied when manufacturing the control unit:

- » EMC-Directive 2014/30/EU Module A
- » Directive 2001/95/EC on general product safety

1.2 Material properties

Control cabinet materials		
Housing	GRP	
	Stainless steel	Option
Display	Plastic	Option

1.3 Pneumatics

Pneumatic hoses	Ø - external	Ø - internal
For compressed air supply	8 mm	6 mm
For control air	6 mm	4 mm
For position feedback	4 mm	2 mm

1.4 Dimensions

Dimensions	Plastic	Stainless steel
Width	300 mm	300 mm
Height	400 mm	400 mm
Depth	250 mm	250 mm

1.5 Environmental conditions

Temperature		
Ambient temperature	0...55 °C	
Transport and storage temperature	-10...60 °C	
Environment		
Relative humidity	10... 95 %	Non-condensing

Protection class		
Housing with switches and LEDs	IP 54	With guard door closed
Housing with display	IP 54	With guard door closed

1.6 Connection values

Electrical connection values		
Voltage supply	24 V DC	30 VA
Input for external contacts	24 V DC	Self-supply for floating contact
Maximum current consumption	1.6 A	
Output for external relay, Cleaning pump I, II and III	24 V DC	Max. 250 mA
Output for status and alarm contacts	24 V DC	Max. 100 mA

1.7 Cleaning valves (optional)

Compressed air	
	<ul style="list-style-type: none"> » According to ISO8573-1:2010 [5:4:4] » Filtered, 40 µm, water and oil-free » 6 bar » No continuous air consumption

1.8 Identification plate

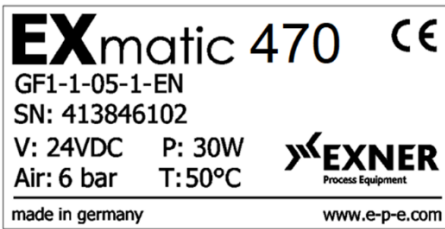


Fig. 1: Identification plate

The identification plate is located on the inside of the cabinet door!

In case of queries, please contact your retailer directly!

2 Product description

2.1 EXmatic 470 electro-pneumatic control unit

External view




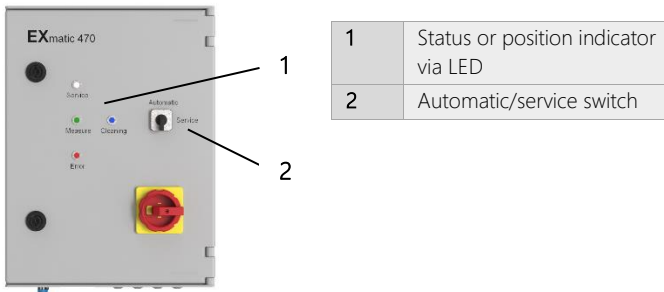


Fig. 2: Probe housing control unit from the outside (with or without a display)

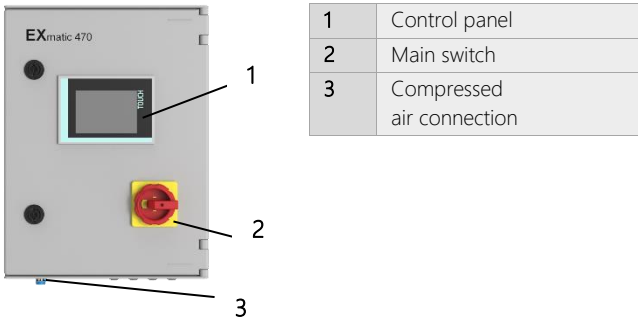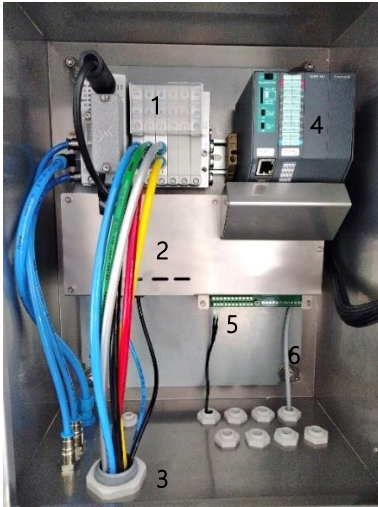

1	Valve manifold
2	Pressure switch
3	Multi-connection hose inlet
4	Control unit (PLC)
5	Connection terminals
6	PE connection

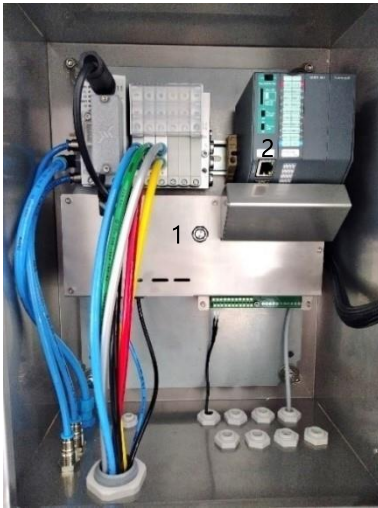

1	Push button (momentary) start/stop for the cleaning programme
2	LAN Port

Fig. 3: Control unit from the inside (with/without display)

Function

The probe housing control unit EXMATIC 470 enables fully automatic control and monitoring of measuring and cleaning cycles of pneumatic retractable probe housing. Cleaning

times, measuring intervals and start times can be parameterised and adjusted to individual requirements.

Input

The control unit monitors the respective position feedback from the retractable probe housing via integrated inputs.

Automatic cleaning can be started via an additional input.

Output

The respective status of the retractable housing and the control unit can be transmitted to a superordinate process control system via four contact outputs.

Retractable probe housing

The retractable probe housing and cleaning valves for control of the cleaning solution are connected to the probe housing control system via pneumatic hoses. This should be realised via the dedicated EXconnect multi-connection hose.

2.2 Process integration

The EXmatic 470 probe housing control unit is supplied with 24V DC and compressed air with a pressure of 6 bar. Connection to the retractable probe housing and the cleaning and drain valves is realised via pneumatic hoses which are bundled in a multi-connection hose.

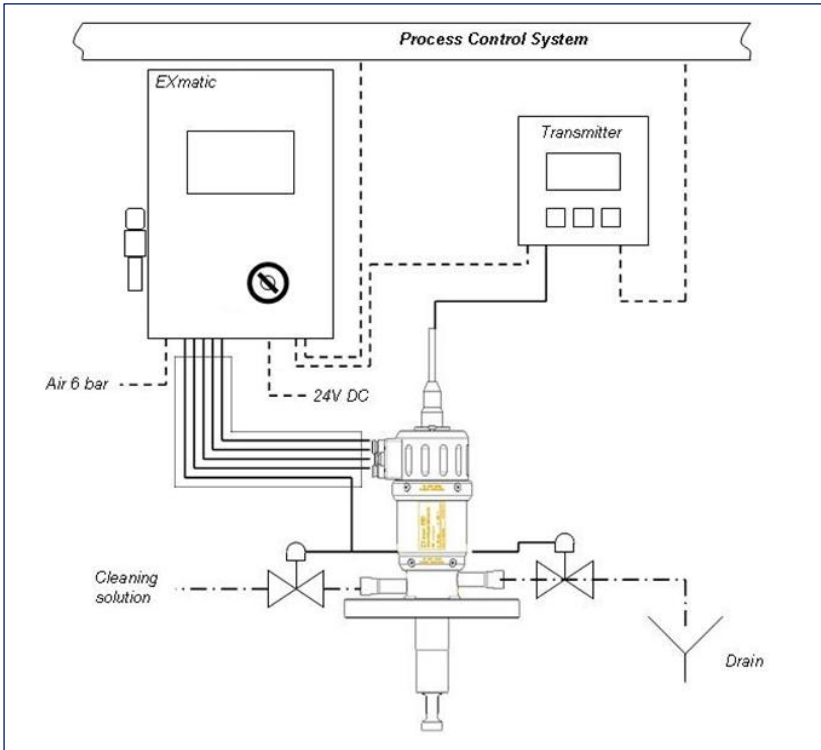


Fig. 4: Process flow

The respective status of the measuring unit (alarm status, measuring status, cleaning status or position service) can be reported via contacts to a superordinate process control system.

Cleaning cycles can be started via an external contact, e.g. from the pH transmitter.

The EXmatic 470 probe housing control unit is fully independent and can be operated from a transmitter or process control system without any connection.

The probe housing control unit features a manual as well as an automatic mode. In manual mode, motion of the retractable probe housing and the individual cleaning valves can be controlled manually. The probe housing control unit without a display provides this function only if the "RemoteStage" software described is used.

In automatic mode, a parameterised cleaning process runs after a cleaning cycle is started. After its completion, the retractable probe housing moves to "Measuring" position.

3 EXmatic 470 order structure

	Code	Housing				
	GF0	Plastic (GRP) without a display				
	GF1	Plastic (GRP) with a display				
	SS0	Stainless steel without a display				
	SS1	Stainless steel with a display				
	XXX	Special version				
		Code	Cleaning			
		1	For one cleaning solution			
		2	For two cleaning solutions			
		3	For three cleaning solutions			
		X	Special version			
		Code	Multi-connection hose length			
		00	Without multi-connection hose			
		03	3 metres			
		05	5 metres			
		10	10 metres			
		XX	Special version			
		Code	Compressed air maintenance unit			
		0	Without			
		1	With an integrated maintenance unit			
		X	Special version			
		Code	Interface			
		EN	Without			
		XX	Special version			
EXmatic 470						Order code

4 Spare parts and accessories

Spare parts		
EXmatic 470	Spare parts	Order number
	Diaphragm valve PTFE/EPDM DN12 PN6 for cleaning solution	2-095-70-001
	Pilot control valve 5/2-way monostable, 24 V DC	2-091-10-003
	Pilot control valve 2x3/2-way NC, 24 V DC	2-091-10-004
	Pressure switch 0-10 bar Ø 4 mm PNP	2-096-00-002

Accessories		
Control cabinet	Accessories	Order number
	Wall mounting, plastic control cabinet	2-083-73-001
	Wall mounting, stainless steel control cabinet	2-083-73-002
	Pole mounting (plastic/stainless steel)	2-083-70-003
Diaphragm valves	Accessories	Order number
PVDF/EPDM G 3/8", DN12, PN6, NC	Cleaning valve set for one cleaning valve and one drain valve	2-095-70-002
	Cleaning valve set for two cleaning valves and one drain valve	2-095-70-003
	Cleaning valve set for three cleaning valves and one drain valve	2-095-70-004
Maintenance unit	Accessories	Order number
	Compressed air maintenance unit	2-078-73-001

NOTE

When ordering spare parts and accessories, please specify the serial number of your unit.

5 Certificates and compliance

EU-Declaration of conformity

for
Control unit EXmatic470

We declare under our sole responsibility that the product, to which this declaration relates, is in conformity with the following standards and the normative documents:

EU- Directive	harmonized standards
EMC-Directive 2014/30/EU Module A	DIN EN 61326-1:2013 IEC 61326-1: 2020 Emission: Class B Immunity: Industrial environment
Directive 2001/95/EC on general product safety	DIN EN 61010-1:2020-03
RoHS 2 Directive 2011/65/EU + Delegated Directive 2015/863/EU	DIN EN 63000:2019-05

This declaration applies to all identical specimens of the product, which are manufactured according to the development-, design- and manufacturing drawings and descriptions, which are part of this declaration.

This declaration is given by the manufacturer.

Name of company:
Address:

Exner Process Equipment GmbH
Carl-Metz-Straße 26
D-76275 Ettlingen

Germany

E. K. J. P.
Place

26.04.2022
Date

M. T.
Michael Tottewitz
General Manager






Exner Process Equipment GmbH
Carl-Metz-Str. 26
D-76275 Ettlingen
Germany

tel +49 (0)7243-94 54 29-0
fax +49 (0)7243-94 54 29-99
mail info@e-p-e.de

www.e-p-e.com